



# Welcome

KANE452NO

Flue Gas Analyser with  
direct CO<sub>2</sub> measurement,  
CO sensor 'over-range'  
protection & low range  
NO sensor

Quick reference guide




# Hello KANE452NO getting started

- 1 Know your KANE452NO
- 2 Connections
- 3 Before use
- 4 Product registration

Please register your analyser at [www.kane.co.uk](http://www.kane.co.uk) & download the full instruction manual from the product selector


**PLEASE READ ALL SAFETY WARNINGS IN THE MANUAL**

## 1 Know your KANE452NO

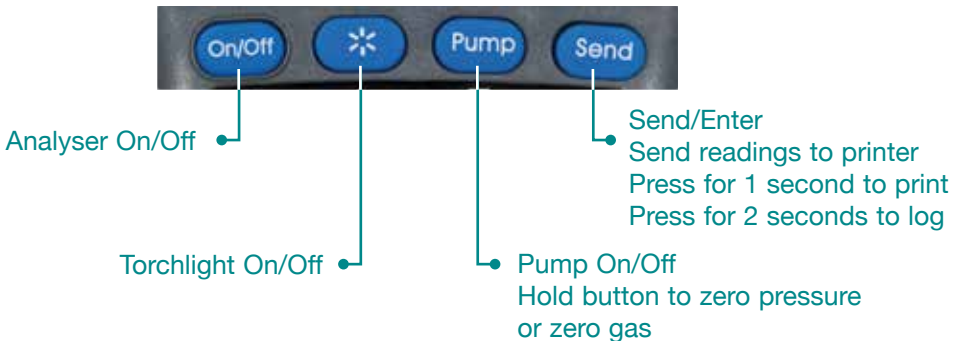

## 2

### Connections

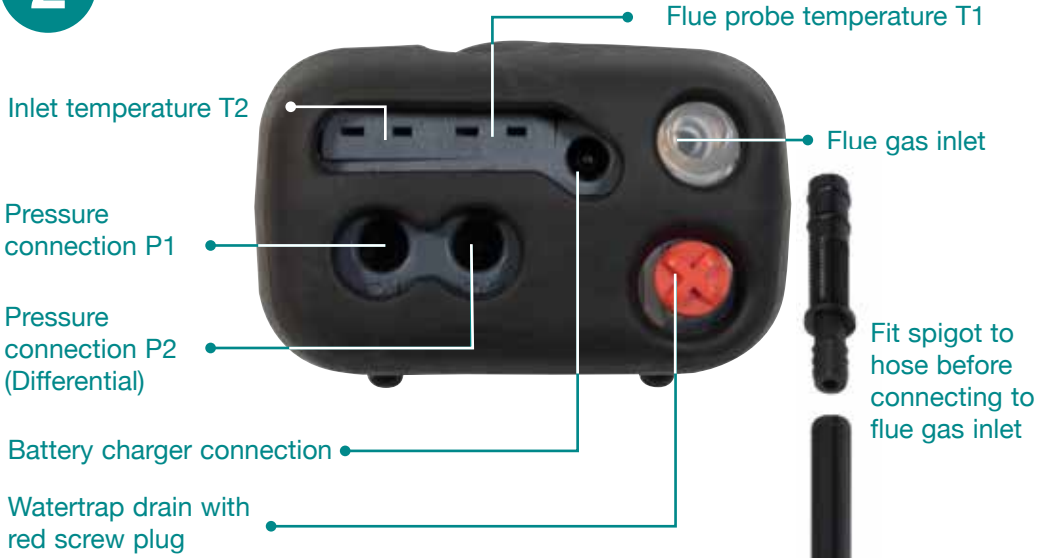

## 3

### Before use

#### Check

Particle filter is not dirty; Water trap & flue probe are empty of water; Water trap & red screw plug are fitted to analyser; Flue probe hose is connected to flue gas inlet; Flue probe temperature plug is connected to T1 temperature connection

#### Fresh air purge

Position flue probe in fresh air & press "On/Off"  
Analyser auto-calibrates within 90 seconds  
Select "Ratio" on dial. In fresh air CO reading = 0ppm  
Select "O<sub>2</sub>/Eff" on dial. In fresh air O<sub>2</sub> reading = 20.9%  
Select "Status" on dial to view

#### For best pressure sensor accuracy

Switch analyser on for 5 minutes to let temperature stabilise  
Zero pressure sensor when analyser in exact position it will be used

#### To charge NiMH rechargeable batteries

Switch off  
Connect the charger; charging indicator illuminates  
Display shows "BATTERY CHARGING" if batteries need charging

# 4

## Please register

We really want you to register your Kane analyser at [www.kane.co.uk](http://www.kane.co.uk)

Benefits include:



Download full instruction manual



Automatic reminder when time to Service – Calibrate – Recertify



Fixed prices always visible



Simple online procedure to arrange to Service - Calibrate - Recertify ensures fastest turnaround times possible



Easy access to your calibration certificate & service history



Easy to report your analyser stolen



Product specific information & resources in one place